

Tack Endovascular System®

Below-the-Knee (BTK)




The Tack Endovascular System is a first-of-its kind dissection repair device that is purpose-built to provide precision treatment of peripheral arterial dissections following balloon angioplasty in below-the-knee therapeutic interventions.

PRODUCT HIGHLIGHTS

The Tack® implant features **Adaptive Sizing™** which allows the device to adapt to tapering anatomy while maintaining a relatively constant radial force. This means that a single Tack implant can be used across a range of vessel diameters.

- 4F/.014" OTW delivery system
- 150cm working length
- 4 pre-loaded 4F Tack implants
- Self-sizes to tapering vessel diameters from 1.5-4.5mm with a single system
- Accurate (≤ 1 mm) deployment
- Nitinol with gold radiopaque markers

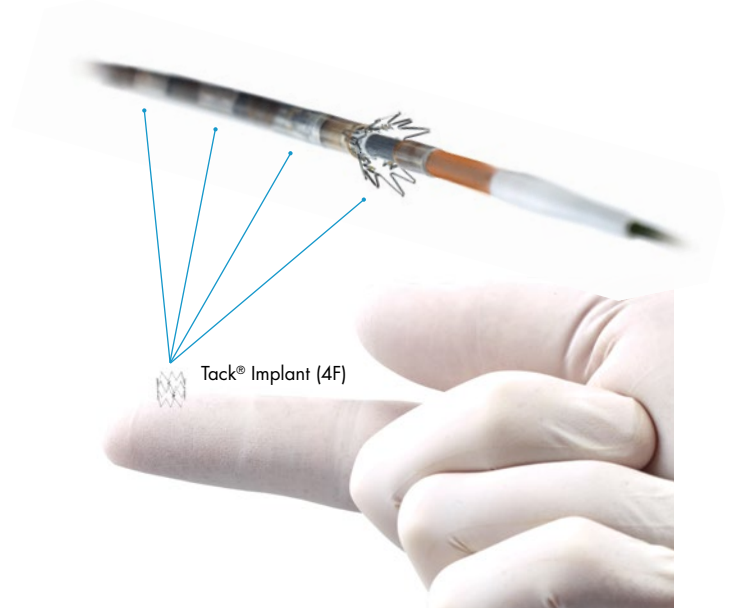

SKU NUMBER	CATHETER LENGTH (CM)	TACK® IMPLANT LENGTH (MM)	NUMBER OF TACKS	TREATMENT RANGE (MM)
154150041	150	6.0	4	1.5-4.5

CONTACT INFORMATION

ORDERING

Tel: +1 (800) 865-0214 | Fax: +1 (484) 816-7130
email: cs@intactvascular.com

GENERAL QUESTIONS

Intact Vascular Customer Service:

email: cs@intactvascular.com

INTENDED USE:

The Tack Endovascular System (4F, 1.5-4.5mm) is intended for use in mid/distal popliteal, tibial and peroneal arteries, ranging in diameter from 1.5 mm to 4.5 mm, for the repair of post percutaneous transluminal balloon angioplasty (PTA) dissection(s).

CONTRAINDICATIONS FOR USE:

The Tack Endovascular System is contraindicated for the following:

1. Patients with residual stenosis in the treated segment equal to or greater than 30% after PTA.
2. Tortuous vascular anatomy significant enough to prevent safe introduction and passage of the device.
3. Patients with a known hypersensitivity to nickel-titanium alloy (Nitinol).
4. Patients unable to receive standard medication used for interventional procedures such as anticoagulants, contrast agents and antiplatelet therapy.

Prior to using the Tack Endovascular System, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use.

Tack Endovascular System® is CE Mark authorized under EC Directive 93/42/EEC.
Adaptive Sizing™ is a trademark of Intact Vascular, Inc.
Tack Endovascular System® and Tack® are registered trademarks of Intact Vascular, Inc.
Copyright © 2020. All rights reserved.

MKT-0250 Rev 01 US 042020

Intact Vascular, Inc. | 1285 Drummers Lane, Suite 200 | Wayne, PA 19087
Tel: 484.253.1048 | Fax: 484.253.1047 | email: info@intactvascular.com

